

FIG.1 PRIOR ART

- 150: MEASURING APPARATUS
- 154: INVERTED FLUORESCENCE MICROSCOPE
- 153: LIGHT SOURCE
- 155: PHOTODIODE
- 156: CONTROL MEANS
- 157: LIVING TISSUES TO BE MEASURED
- 158: DICHOIC MIRROR

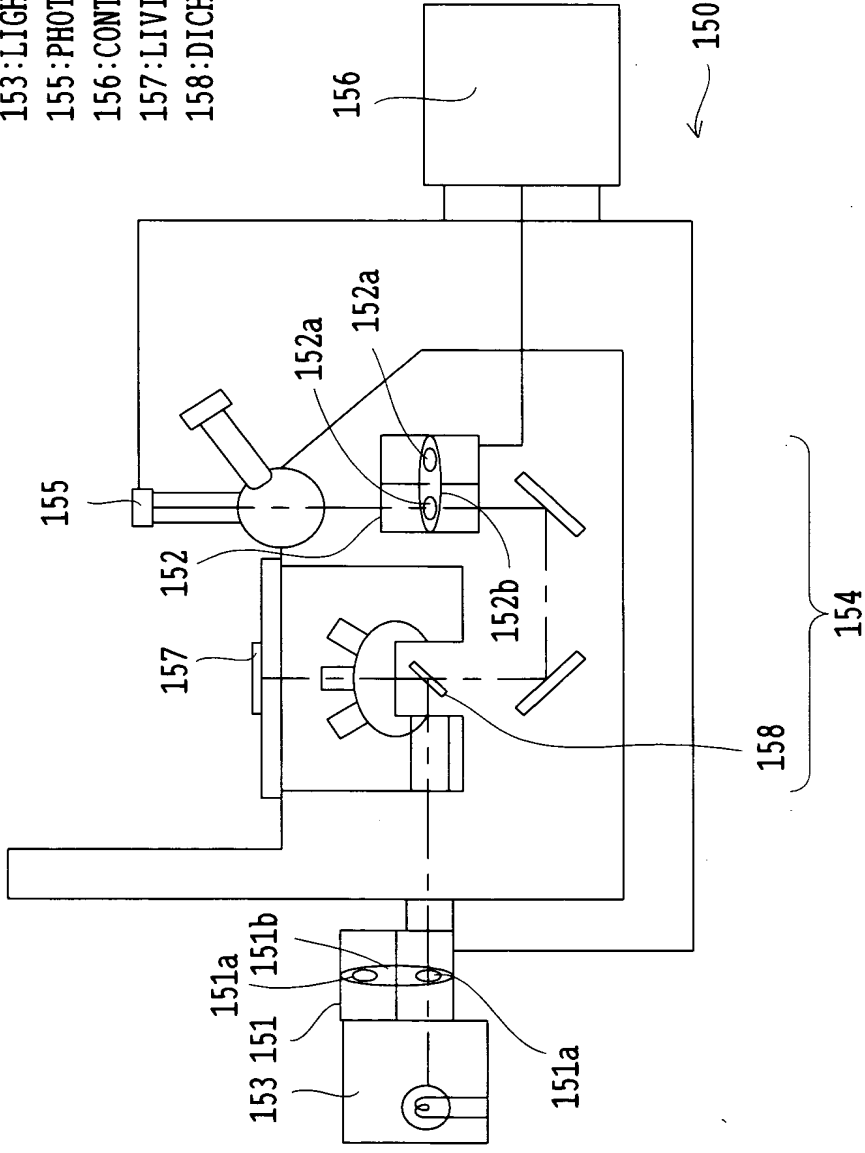


FIG. 2 PRIOR ART

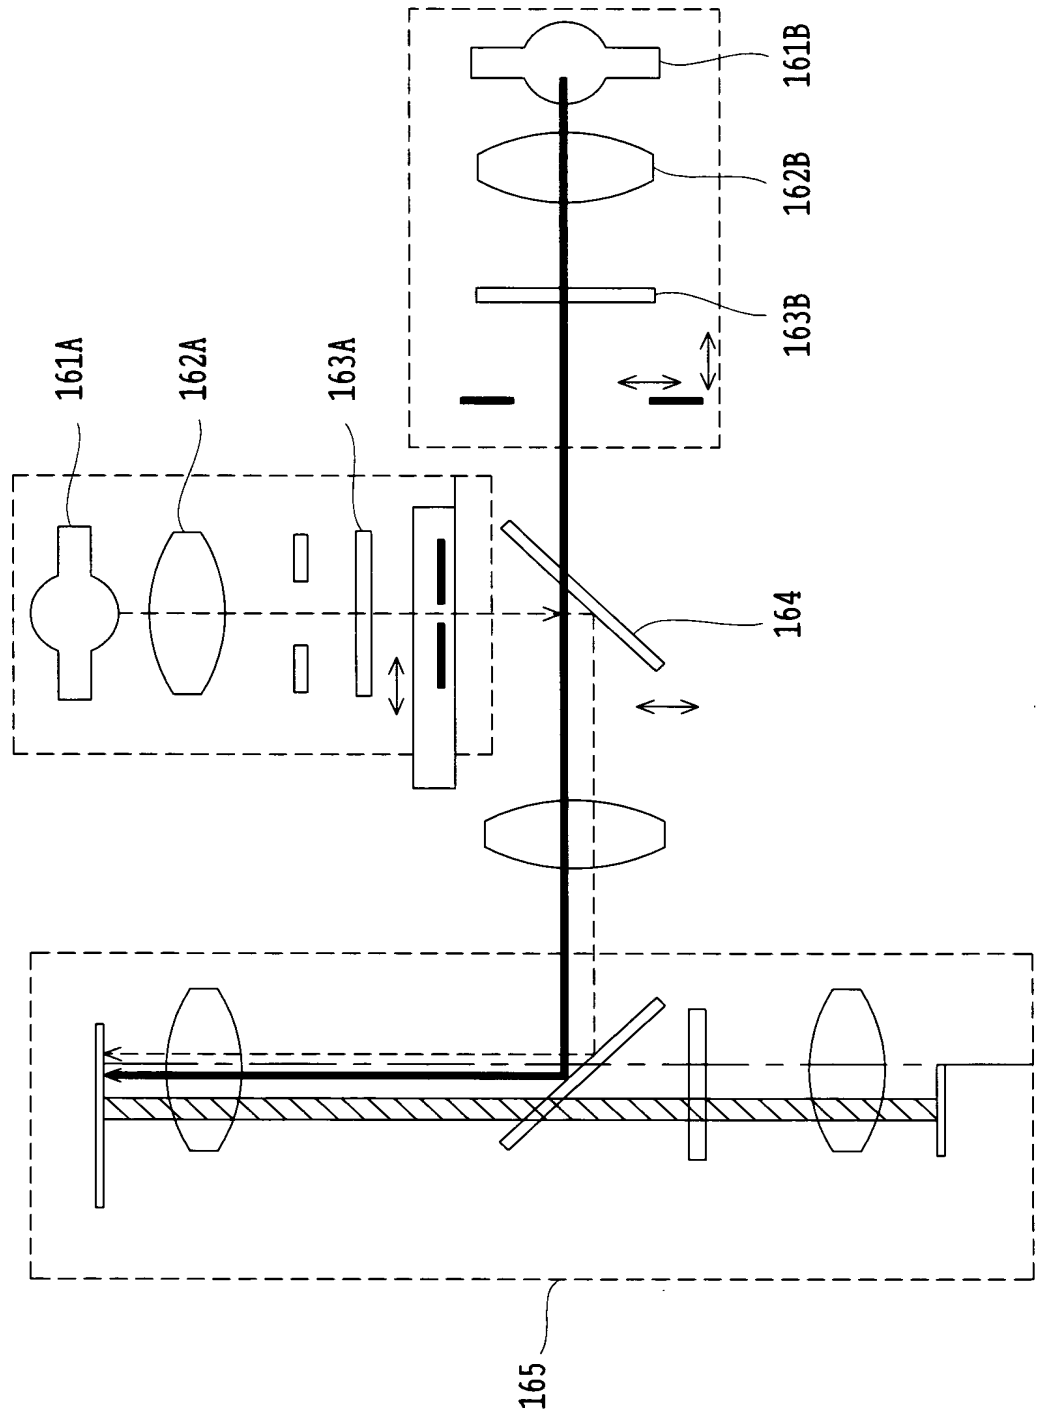


FIG. 3 PRIOR ART

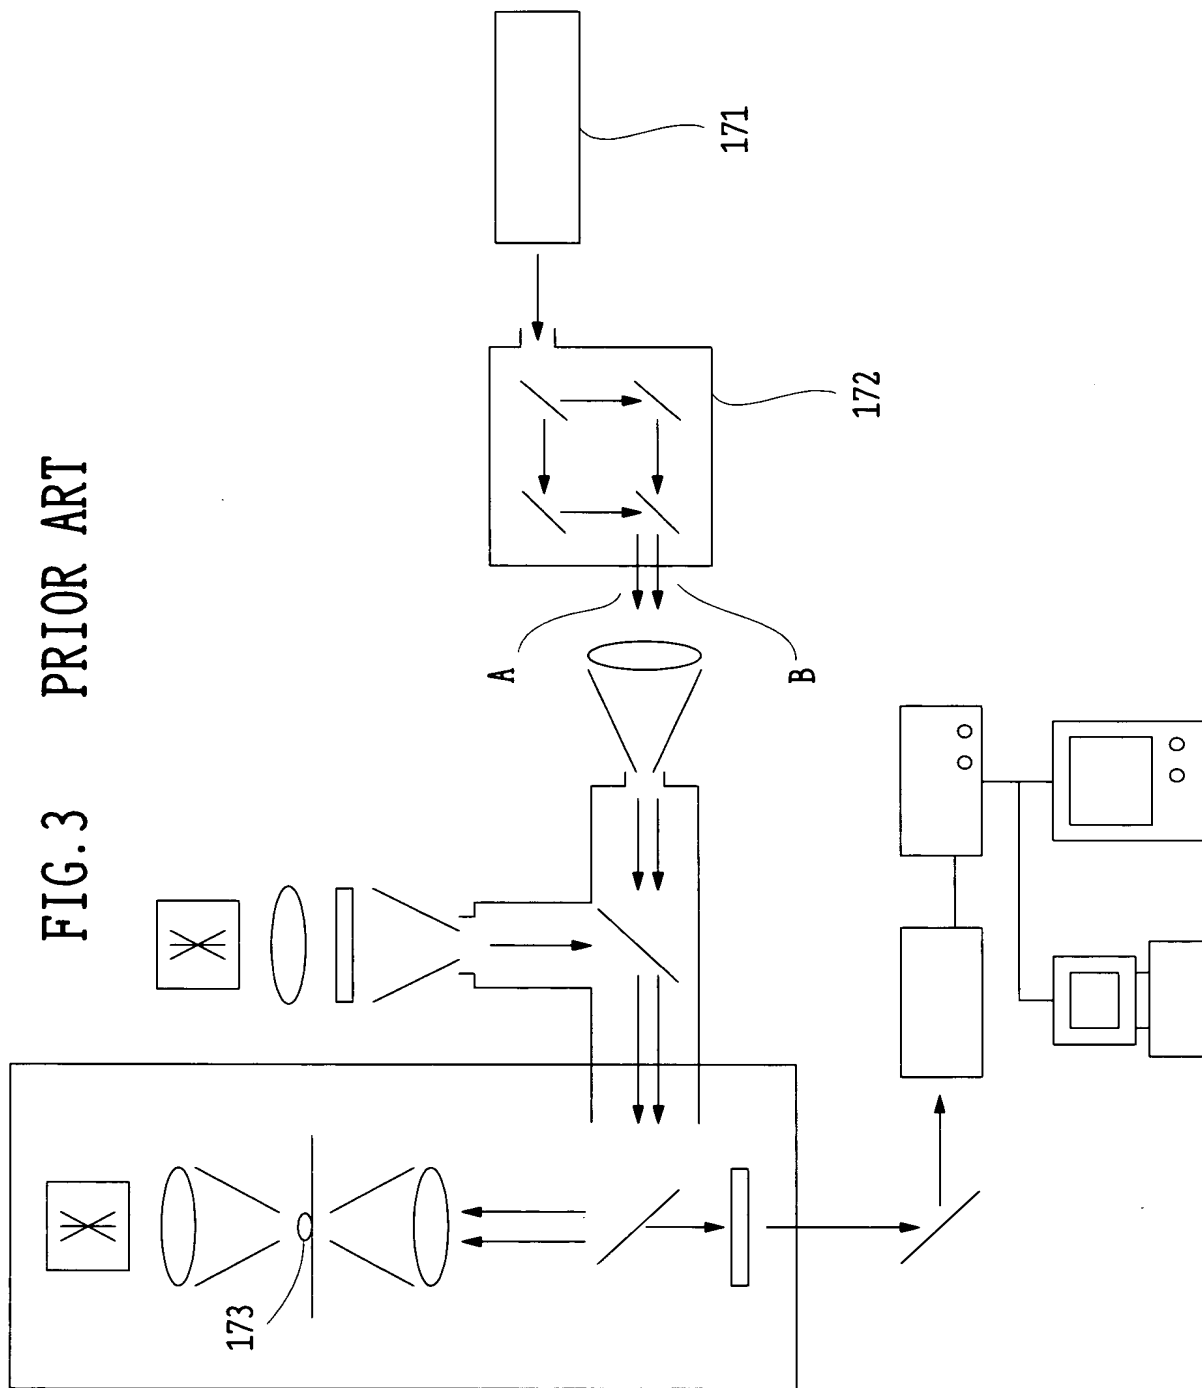


FIG. 4

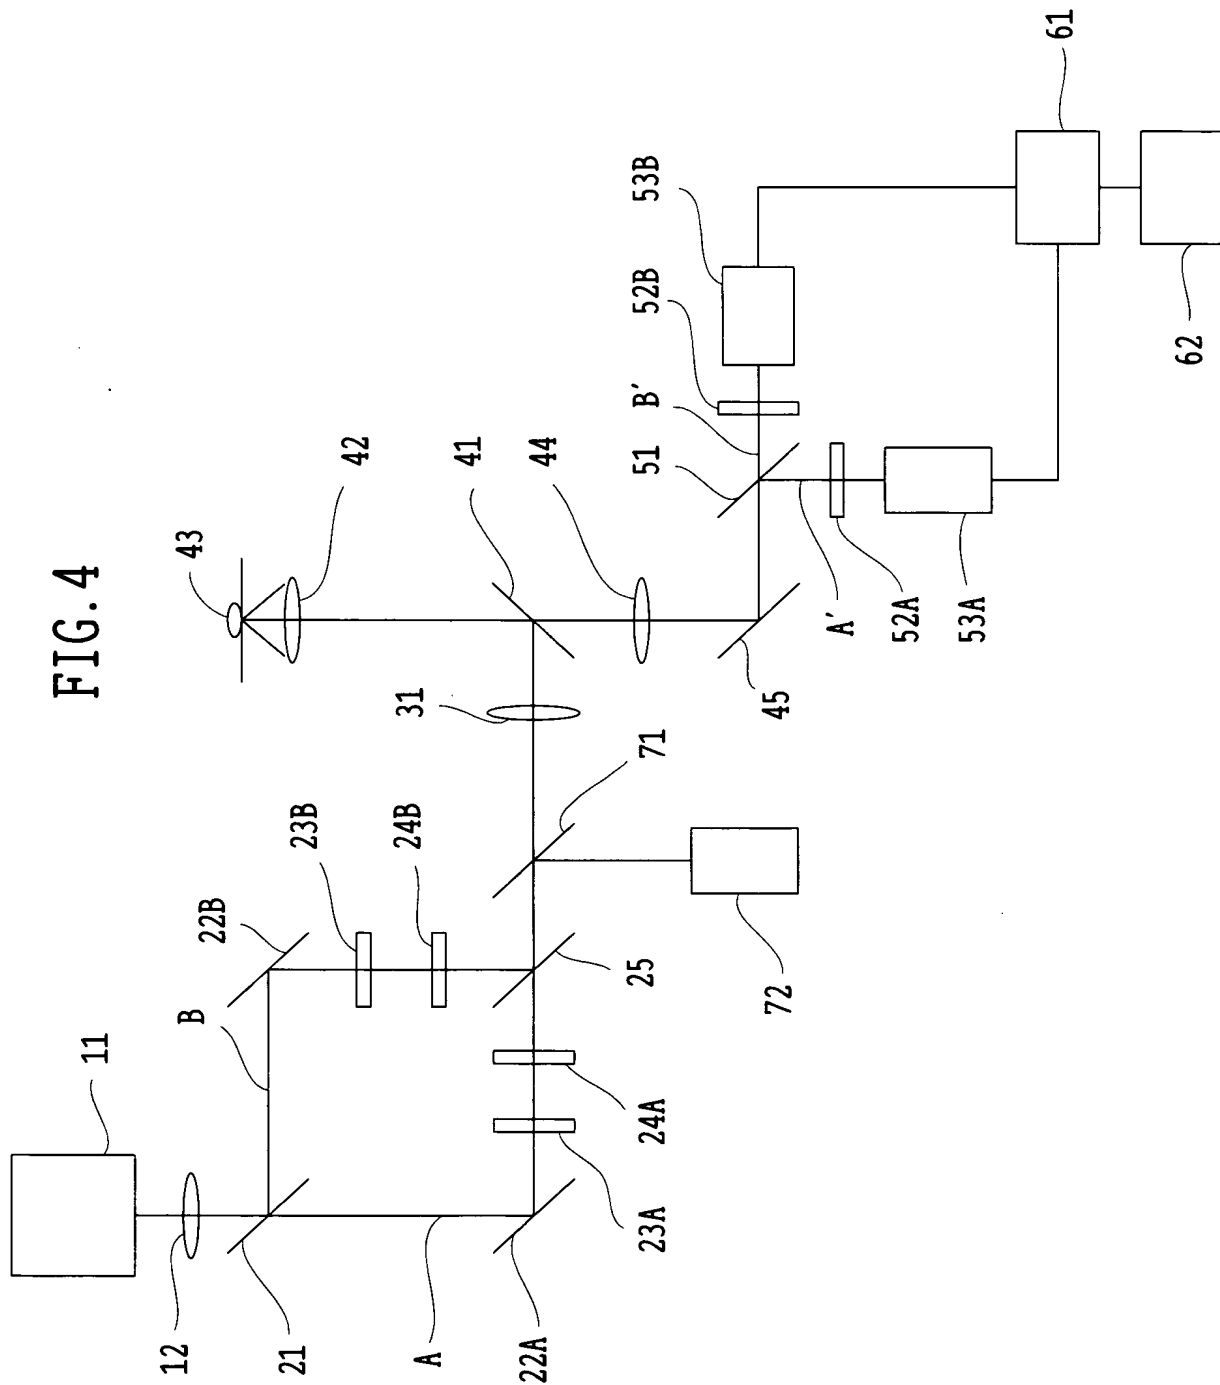


FIG. 5

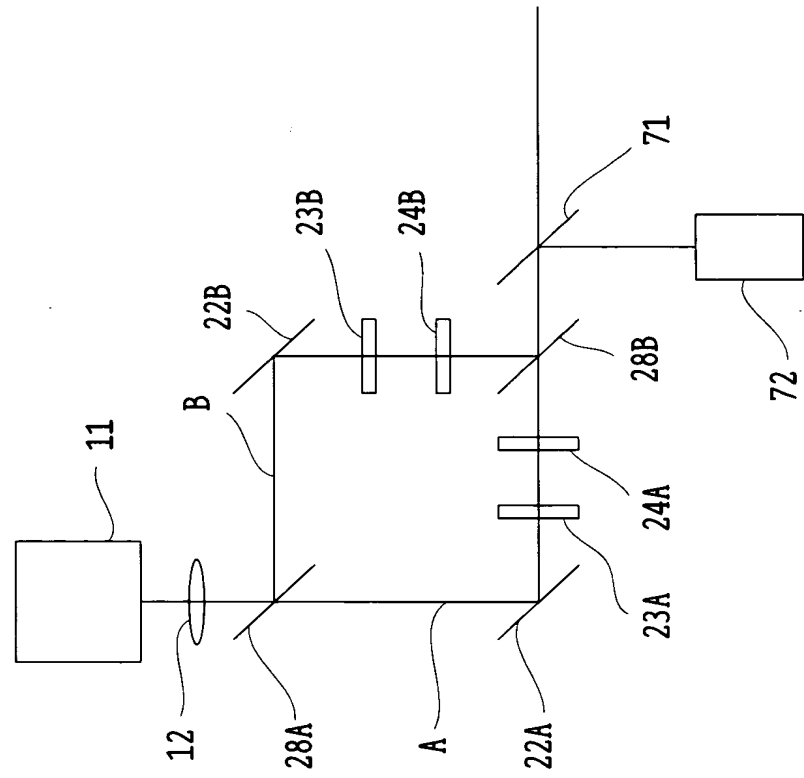


FIG. 6

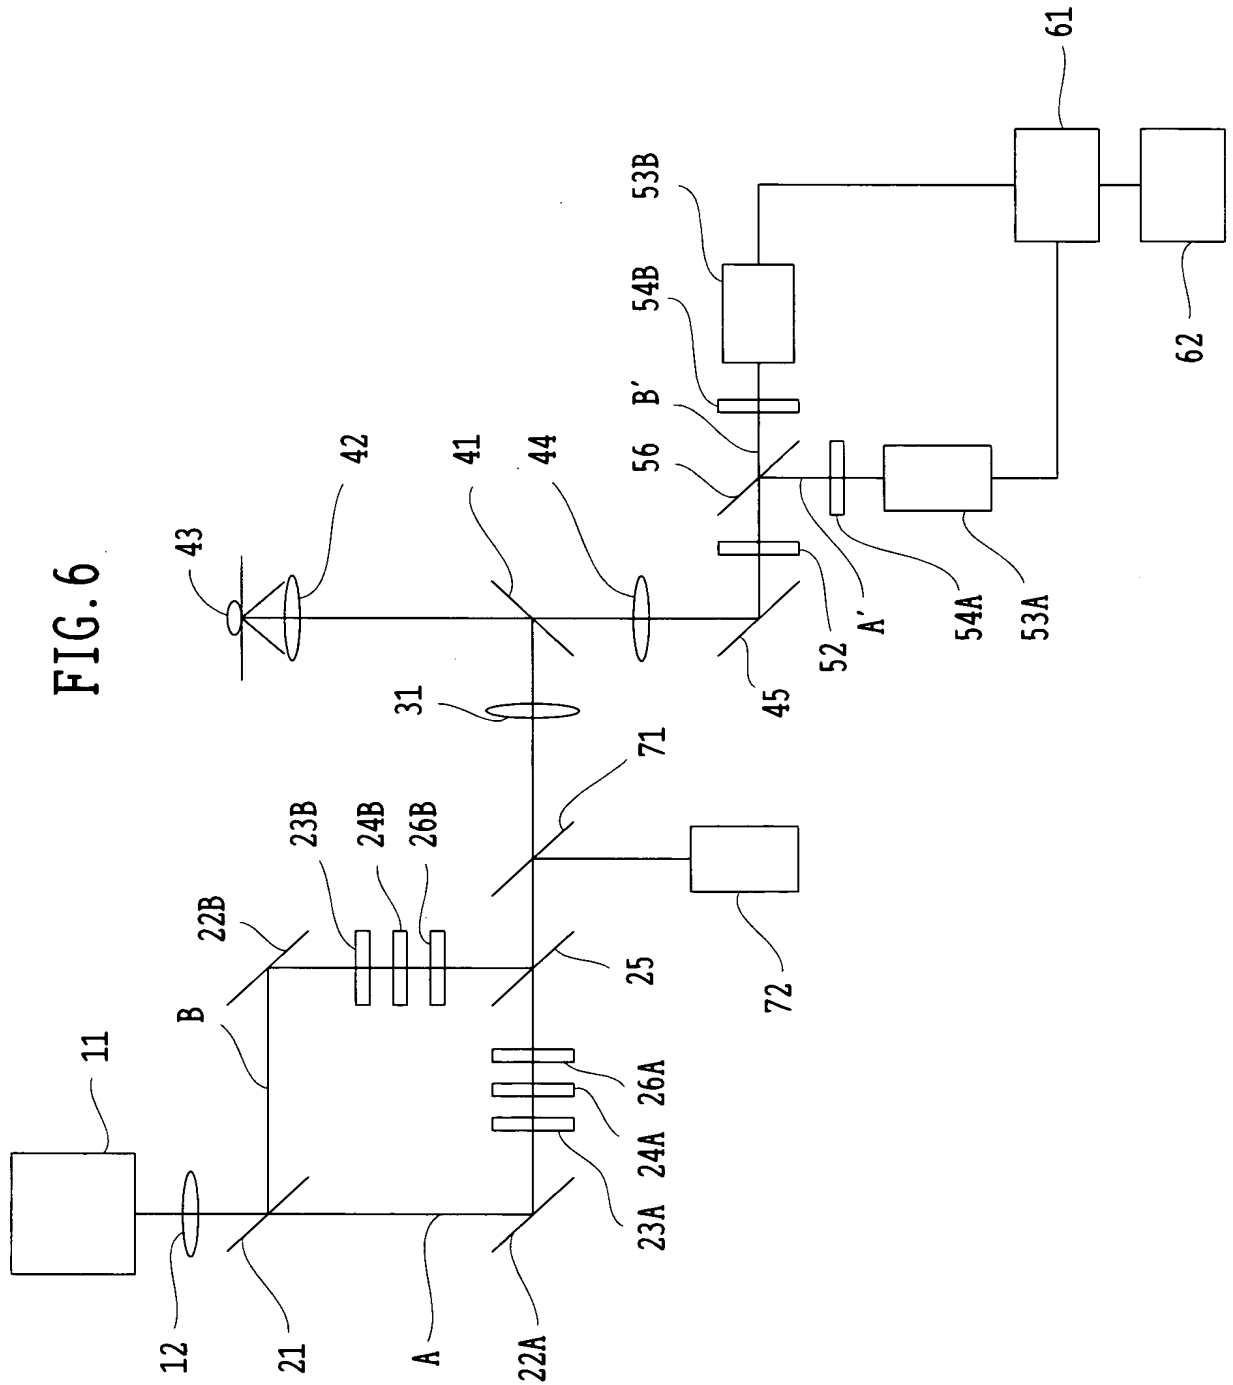


FIG. 7

